


ACCOLADE™

Pacing Systems

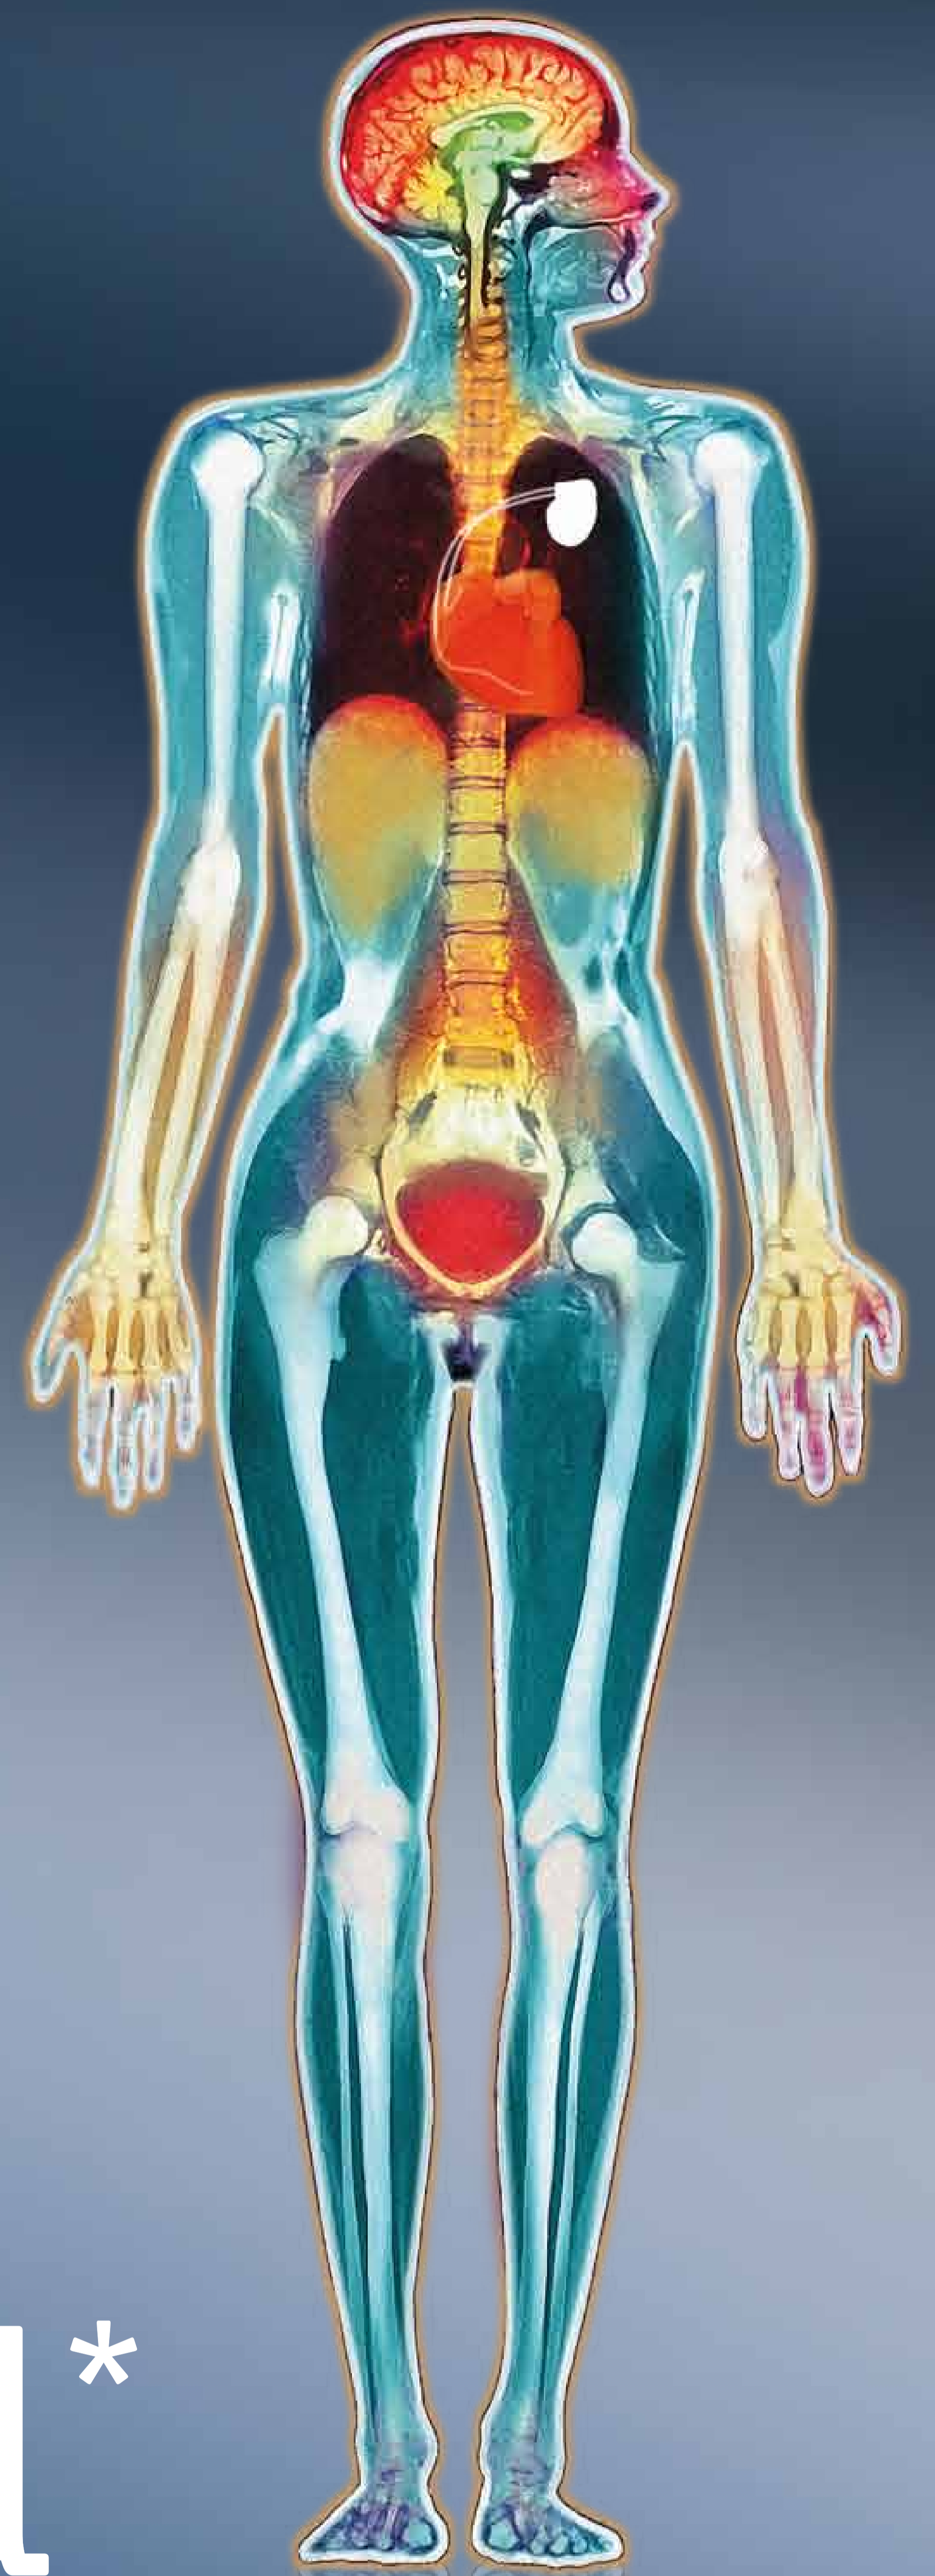

MRI Unlimited*

*Under the Conditions of Use described in IMAGEREADY™ MR Conditional Pacing System Technical Guide. Only specific combinations of pulse generators and leads constitute an ImageReady™ Pacing System. Consult the Technical Guide to distinguish between combinations that are valid for use with ONLY 1.5T scanners and combinations that are valid for use with both 1.5T and 3T scanners. IMAGEREADY™ MR Conditional Pacing System Technical Guide. 359259-018 EN Europe 2014-02.

All cited trademarks are the property of their respective owners. CAUTION: The law restricts these devices to sales by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labelling supplied with each device. Information for the use only in countries with applicable health authority product registrations.

CRM-303105-AA MAR2015 © 2015 Boston Scientific Corporation or its affiliates. All rights reserved.